


# TECNIS Odyssey™ IOL

with TECNIS SIMPLICITY™ Delivery System

Model DRT100-DRT375

Toric II

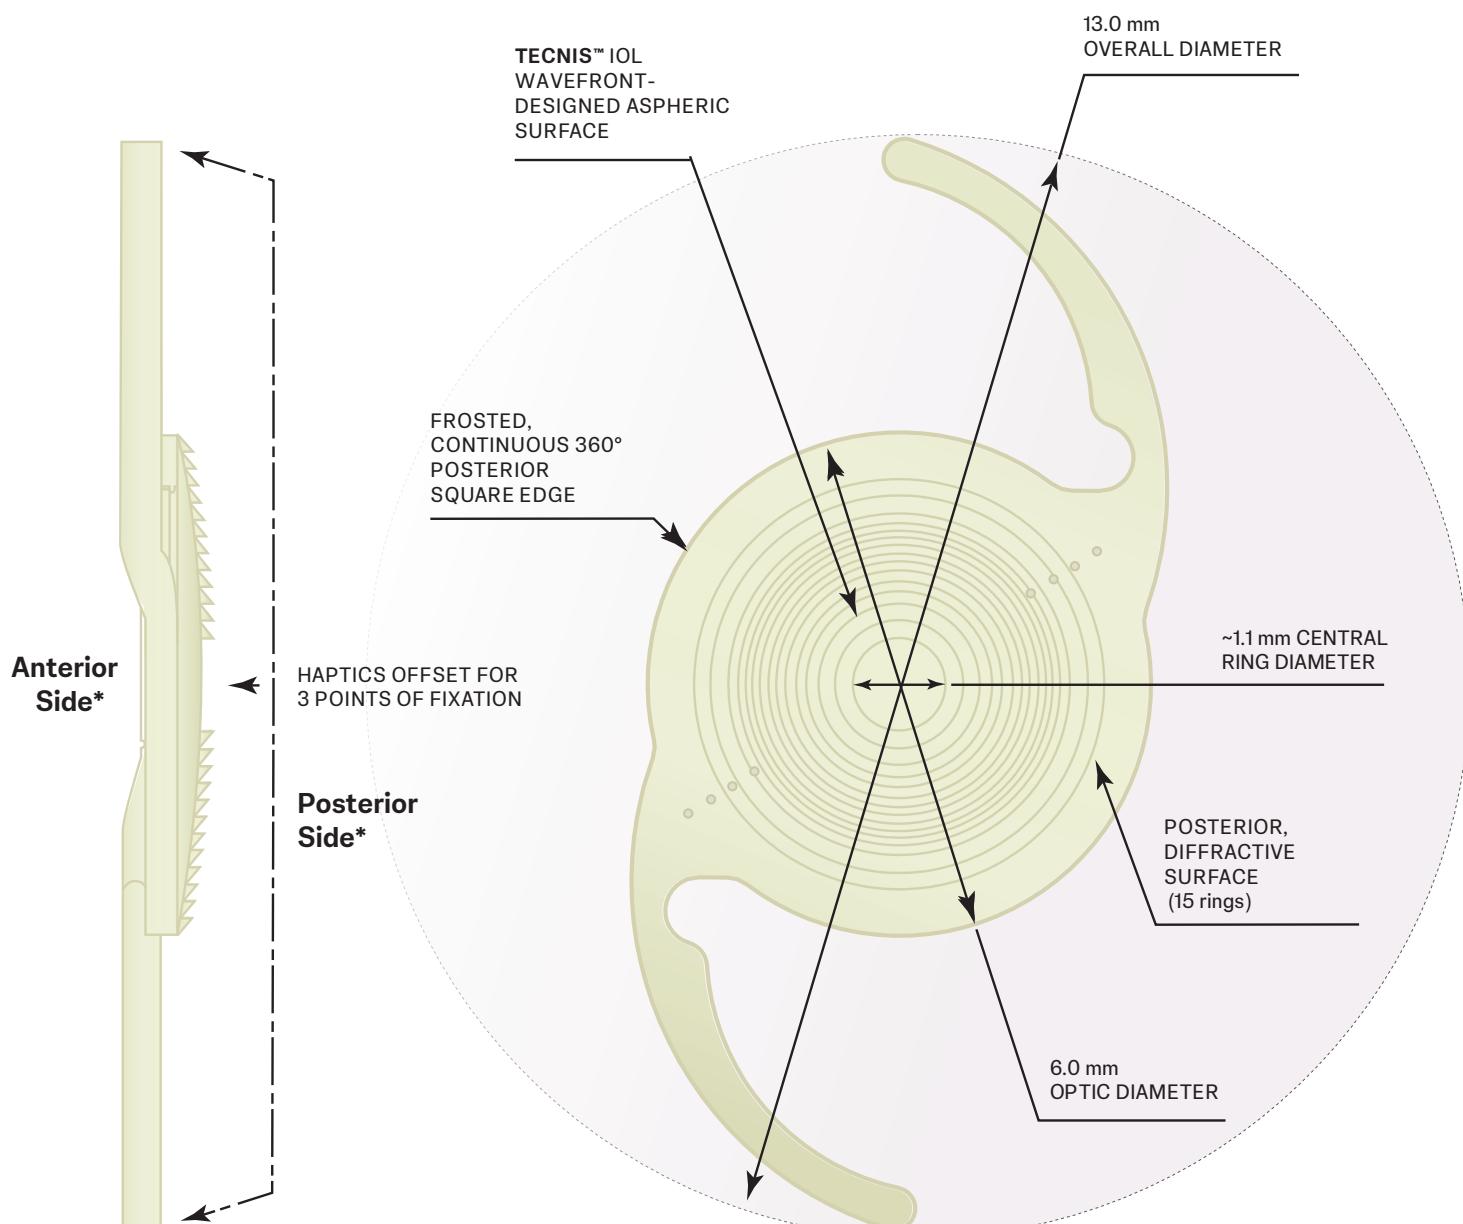

\*Image for illustration purposes only.

Johnson&Johnson

Vision

# TECNIS Odyssey™ IOL

with TECNIS SIMPLICITY™ Delivery System

Toric II

Model DRT100-DRT375



## OPTICAL CHARACTERISTICS<sup>1</sup>

Model Numbers:	DRT100	DRT150	DRT225	DRT300	DRT375
Cylinder Powers - IOL Plane	1.00 D	1.50 D	2.25 D	3.00 D	3.75 D
Cylinder Powers - Corneal Plane	0.69 D	1.03 D	1.54 D	2.06 D	2.57 D
SE Powers:	+5.0 D to +34.0 D in 0.5 diopter increments				
Diameter:	6.0 mm				
Center Thickness:	0.7 mm (20.0 D)				
Shape:	Biconvex, wavefront-designed anterior aspheric surface, proprietary posterior diffractive surface to provide a full range of vision				
Material:	UV-absorbing hydrophobic acrylic with violet-light filter				
Refractive Index:	1.47 at 35 ° C				
Edge Design:	ProTEC frosted, continuous 360° posterior square edge				
Achromatic Technology:	Proprietary technology for chromatic aberration correction to enhance contrast				

## BIOMETRY\*

## CONTACT ULTRASOUND<sup>†</sup>

## OPTICAL<sup>††</sup>

A-constant:	118.8	119.3
AC Depth:	5.4 mm	5.7 mm
Surgeon Factor: <sup>2</sup>	1.68 mm	1.96 mm

## HAPTIC CHARACTERISTICS<sup>1</sup>

Overall Diameter:	13.0 mm
Thickness:	0.46 mm
Style:	C
Material:	UV-absorbing hydrophobic acrylic with violet-light filter
Design:	TRI-FIX, Haptics offset from optics; 1-piece lens

## Preloaded TECNIS SIMPLICITY™ Delivery System

\* Values theoretically derived for a typical 20.0 D lens. Johnson & Johnson recommends that surgeons personalize their A-constant based on their surgical techniques and equipment, experience with the lens model and postoperative results.

<sup>†</sup> IOL constants have been theoretically derived for contact ultrasound.

<sup>††</sup> IOL constants have been derived from clinical evaluation results of the TECNIS™ 1-Piece IOL Platform.

For optimal results, utilize the TECNIS™ Toric IOL calculator at [www.tecnistoriccalc.com](http://www.tecnistoriccalc.com) to determine the appropriate Toric model and power.

### References:

1. TECNIS Odyssey™ Toric II IOL with TECNIS SIMPLICITY™ Delivery System, Model DRT (DRT150-DRT375), Z311983E, current revision.
2. Holladay JT. International Intraocular Lens & Implant Registry 2003. *J Cataract Refract Surg*. 2003; 29:176-197. REF2016CT0151.

For healthcare professionals only. Please reference the Instructions for Use for a complete list of Indications and Important Safety Information and contact our specialists in case of any question.

© Johnson & Johnson and its affiliates 2024 | 2024PP13664